



#1 in Knee Bracing

CCMI Mark III

3151 Scott Street
Vista, CA 92081-8553
USA

Tel: (800) 336-6569
www.djoglobal.com

Fax To: (800) 457-4221

Email To: defiance.help@djoglobal.com

BILL TO:

Account Name: _____
Account #: _____ P.O. #: _____
Contact: _____ Phone: _____
Address: _____
City: _____ State: _____ Zip: _____

SHIPPING INFORMATION: Same as "BILL TO"

Name: _____
Address: _____
City: _____ State: _____ Zip: _____
 UPS Red (overnight) UPS Blue (2 day air)
 UPS 3 Day UPS Ground Other _____

PRODUCT SELECTION: CCMI Mark III

Frame: DEFIANCE® III DEFIANCE® Football/Contact

Hinge:

- FourcePoint™ (ACL only)
- FourcePoint™ Plus (ACL only)
- Female Fource™ (ACL only)
- Low Profile (Standard)
- DropLock (CI only)
- Elbow (CI only)
- Adjustable OA

Recommended Football Options

- Swooping Thigh
 - FourcePoint™ Plus Hinge
 - Chamois Liners/Pads
 - Reinforced Carbon Composite Frame
 - Metal Caps — Power Caps
 - Square Strap Ends
 - Player Last Name, First Initial
- _____
- School/Team Color: _____

Strapping:

- ACL PCL CI

OA Affected Compartment: Medial Lateral


Degrees of Correction: _____ (1° to 7°) (Standard= 3°)

FOR DJO USE ONLY:

Order #: _____
Brace #: _____

PATIENT INFORMATION:

Name: _____
Age: _____ Height: _____ Weight: _____
Knee Measurement: Right Left Reverse
Measured By: _____
 New Brace Remeasurement/Repair Refurbish

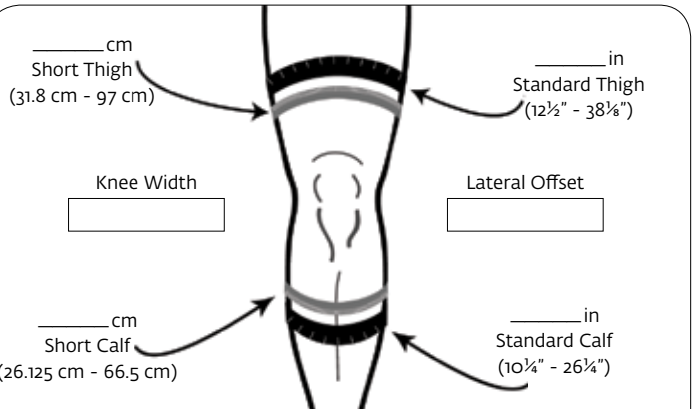

Note: Check both short and standard measurements for ski boot option. Best to measure with Ski Boot On.

NON-METALLIC COLORS:

- Matte Black Neon Pink Neon Yellow Neon Orange
- Black Red Purple Pink
- White Blue Light Blue Yellow
- Green Orange Tan Red, White, Blue

METALLIC COLORS:

- Black Red Purple Pink
- Navy Dark Blue Bright Blue Gold
- Green Orange White Silver

MULTIPLE COLORS:

Thigh Frame: _____
Calf Frame: _____
Fade (non-metallic colors only): Yes No

GRAPHICS (extra charge):

- Tiger Red Tiger Orange Carbon Fiber
- Snake Camouflage
- Stars & Stripes (non-metallic) Stars & Stripes (metallic)

FEATURES (*standard option on DEFIANCE® III):

- Suede Liners/Pads
- Chamois Liners/Pads
- Swooping Thigh (not available on short thigh)*
- Swiveling Strap Tabs*
- Metal Caps - PowerCaps (recommended for contact sports)
- Reinforced Carbon Composite Frame
- Legend Strap Ends
- Installed Extension Stop: 0° 10° 20° 30° 40° (circle one)
- Installed Flexion Stop: 45° 60° 75° 90° (circle one)
- Neoprene Suspension Strap Kit

ACCESSORIES (extra charge):

- High Strength Stainless Steel Gears Air Condyle Kit
- Full Extension Lockout Stop Foam Condyle Pads
- Lycra® Suspension Sleeve Armor Impact Guard
- Neoprene Suspension Sleeve Pinch Guard (Calf)
- Sports Brace Cover Atrophy Pad Kit
- Sili-Grip Strap Pad Kit Tru-Pull® Advanced
- FourcePoint Hinge Stop Kit


For further instructions, please refer to the CCMI Mark III instruction video and instruction card included with the instrument.

CAUTION!

FEDERAL LAW (U.S.A.) RESTRICTS THIS DEVICE TO SALE BY THE ORDER OF A LICENSED HEALTH CARE PROFESSIONAL

Custom Contour Measuring Instrument - Mark III Use Instructions

NOTICE: For optimum long term fit of the DEFIANCE® or DEFIANCE® III, measurements should be taken when there is no edema or atrophy present.

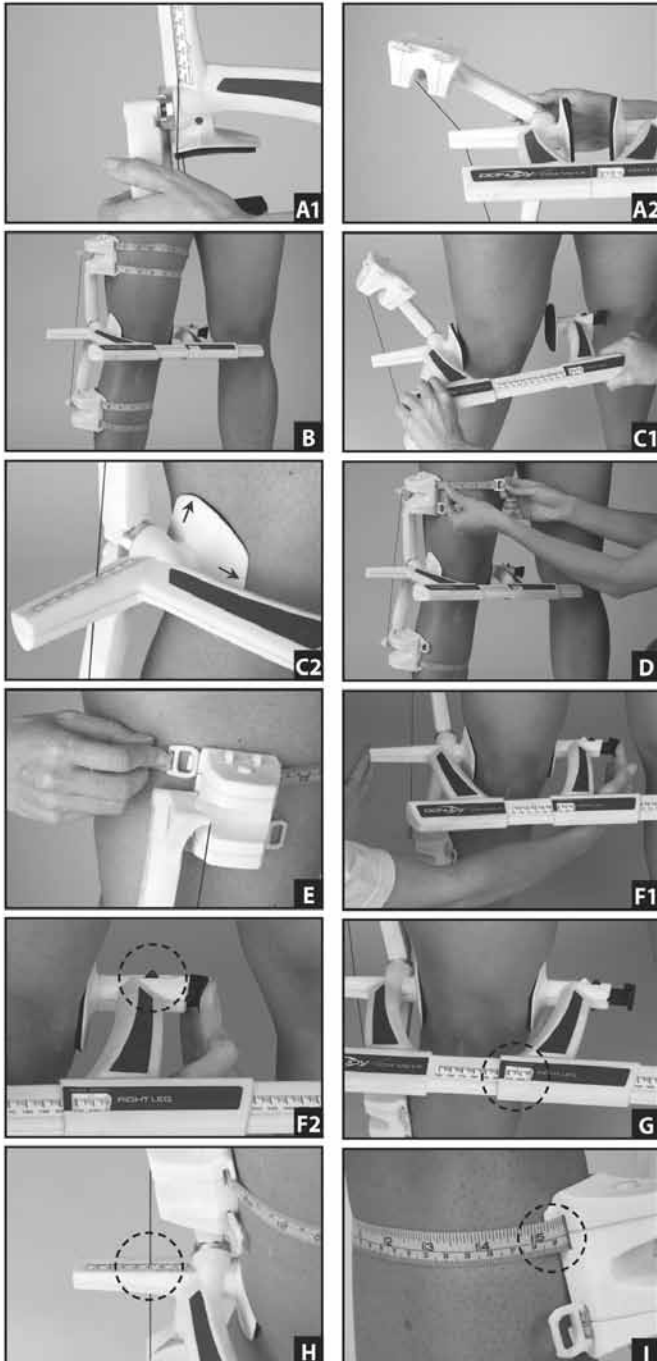

APPLICATION INFORMATION:

1. To unstow, distract and rotate swing arms as shown in figures (A1 and A2).
2. Have the patient stand feet shoulder width apart and knees flexed slightly. Do not allow the knees to flex beyond 15 degrees. Apply the instrument directly to the bare leg. Note: Taking measurements from the uninvolved leg is not recommended because of differences in leg dimensions due to dominance of one leg over the other. See figure B.
3. Distract knee width caliber and position on the patient's knee. Arrows on condyle shells should align with the top of the knee cap and slightly posterior to midline. See figures (C1 and C2).
4. For standard thigh and calf, extend tape measure marked in Inches located distal to knee. Wrap around leg and secure to hook on tape module. Press tape release button to pull tape snug to leg; ensure it is parallel to floor. For short thigh or calf, follow same procedure using Metric measurements. See figure (D and E).
5. To establish proper knee compression for knee width measurement, support lateral side of instrument and press load plunger on medial condyle until triangles are aligned, as shown in figures (F1 and F2).
6. Record knee width on order form. See figure (G.)
7. Record lateral offset on order form. See figure (H).
8. Record thigh and calf circumference on order form. See figure (I).