



#1 in Knee Bracing

### CCMI Mark III

3151 Scott Street  
Vista, CA 92081-8553  
USA

Tel: (800) 336-6569  
www.djoglobal.com

Fax To: (800) 457-4221

Email To: defiance.help@djoglobal.com

#### BILL TO:

Account Name: \_\_\_\_\_  
Account #: \_\_\_\_\_ P.O. #: \_\_\_\_\_  
Contact: \_\_\_\_\_ Phone: \_\_\_\_\_  
Address: \_\_\_\_\_  
City: \_\_\_\_\_ State: \_\_\_\_\_ Zip: \_\_\_\_\_

#### SHIPPING INFORMATION:

Same as "BILL TO"

Name: \_\_\_\_\_  
Address: \_\_\_\_\_  
City: \_\_\_\_\_ State: \_\_\_\_\_ Zip: \_\_\_\_\_  
 UPS Red (overnight)  UPS Blue (2 day air)  
 UPS 3 Day  UPS Ground  Other \_\_\_\_\_

#### PRODUCT SELECTION: CCMI Mark III

Frame:  DEFIANCE® III  DEFIANCE®  Football/Contact

#### Hinge:

- FourcePoint™ (ACL only)
- FourcePoint™ Plus (ACL only)
- Female Fource™ (ACL only)
- Low Profile (Standard)
- DropLock (CI only)
- Elbow (CI only)
- Adjustable OA

#### Recommended Football Options

- Swooping Thigh
  - FourcePoint™ Plus Hinge
  - Chamois Liners/Pads
  - Reinforced Carbon Composite Frame
  - Metal Caps — Power Caps
  - Square Strap Ends
  - Player Last Name, First Initial
- \_\_\_\_\_
- School/Team Color: \_\_\_\_\_

#### Strapping:

ACL  PCL  CI

OA Affected Compartment:  Medial  Lateral


Degrees of Correction: \_\_\_\_\_ (1° to 7°) (Standard= 3°)

#### FOR DJO USE ONLY:

Order #: \_\_\_\_\_  
Brace #: \_\_\_\_\_

#### PATIENT INFORMATION:

Name: \_\_\_\_\_  
Age: \_\_\_\_\_ Height: \_\_\_\_\_ Weight: \_\_\_\_\_  
Knee Measurement:  Right  Left  Reverse  
Measured By: \_\_\_\_\_  
 New Brace  Remeasurement/Repair  Refurbish

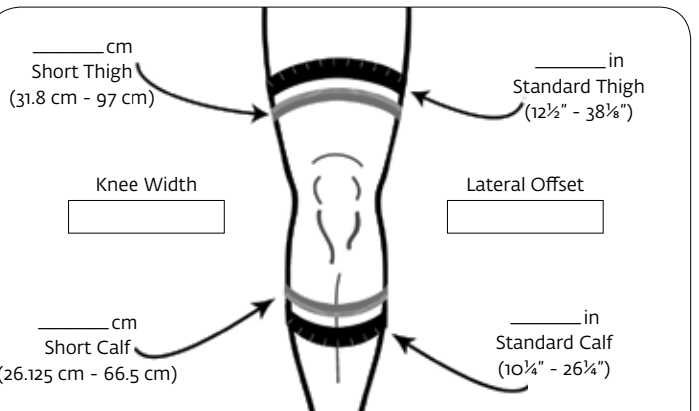

Note: Check both short and standard measurements for ski boot option. Best to measure with Ski Boot On.

#### NON-METALLIC COLORS:

- Matte Black  Neon Pink  Neon Yellow  Neon Orange
- Black  Red  Purple  Pink
- White  Blue  Light Blue  Yellow
- Green  Orange  Tan  Red, White, Blue

#### METALLIC COLORS:

- Black  Red  Purple  Pink
- Navy  Dark Blue  Bright Blue  Gold
- Green  Orange  White  Silver

#### MULTIPLE COLORS:

Thigh Frame: \_\_\_\_\_  
Calf Frame: \_\_\_\_\_  
Fade (non-metallic colors only):  Yes  No

#### GRAPHICS (extra charge):

- Tiger Red  Tiger Orange  Carbon Fiber
- Snake  Camouflage
- Stars & Stripes (non-metallic)  Stars & Stripes (metallic)

#### FEATURES (\*standard option on DEFIANCE® III):

- Suede Liners/Pads
- Chamois Liners/Pads
- Swooping Thigh (not available on short thigh)\*
- Swiveling Strap Tabs\*
- Metal Caps - PowerCaps (recommended for contact sports)
- Reinforced Carbon Composite Frame
- Legend Strap Ends
- Installed Extension Stop: 0° 10° 20° 30° 40° (circle one)
- Installed Flexion Stop: 45° 60° 75° 90° (circle one)
- Neoprene Suspension Strap Kit

#### ACCESSORIES (extra charge):

- High Strength Stainless Steel Gears  Air Condyle Kit
- Full Extension Lockout Stop  Foam Condyle Pads
- Lycra® Suspension Sleeve  Armor Impact Guard
- Neoprene Suspension Sleeve  Pinch Guard (Calf)
- Sports Brace Cover  Atrophy Pad Kit
- Sili-Grip Strap Pad Kit  Tru-Pull® Advanced
- FourcePoint Hinge Stop Kit


For further instructions, please refer to the CCMI Mark III instruction video and instruction card included with the instrument.

## CAUTION!

FEDERAL LAW (U.S.A.) RESTRICTS THIS DEVICE TO SALE BY THE ORDER OF A LICENSED HEALTH CARE PROFESSIONAL

### Custom Contour Measuring Instrument - Mark III Use Instructions

NOTICE: For optimum long term fit of the DEFIANCE® or DEFIANCE® III, measurements should be taken when there is no edema or atrophy present.

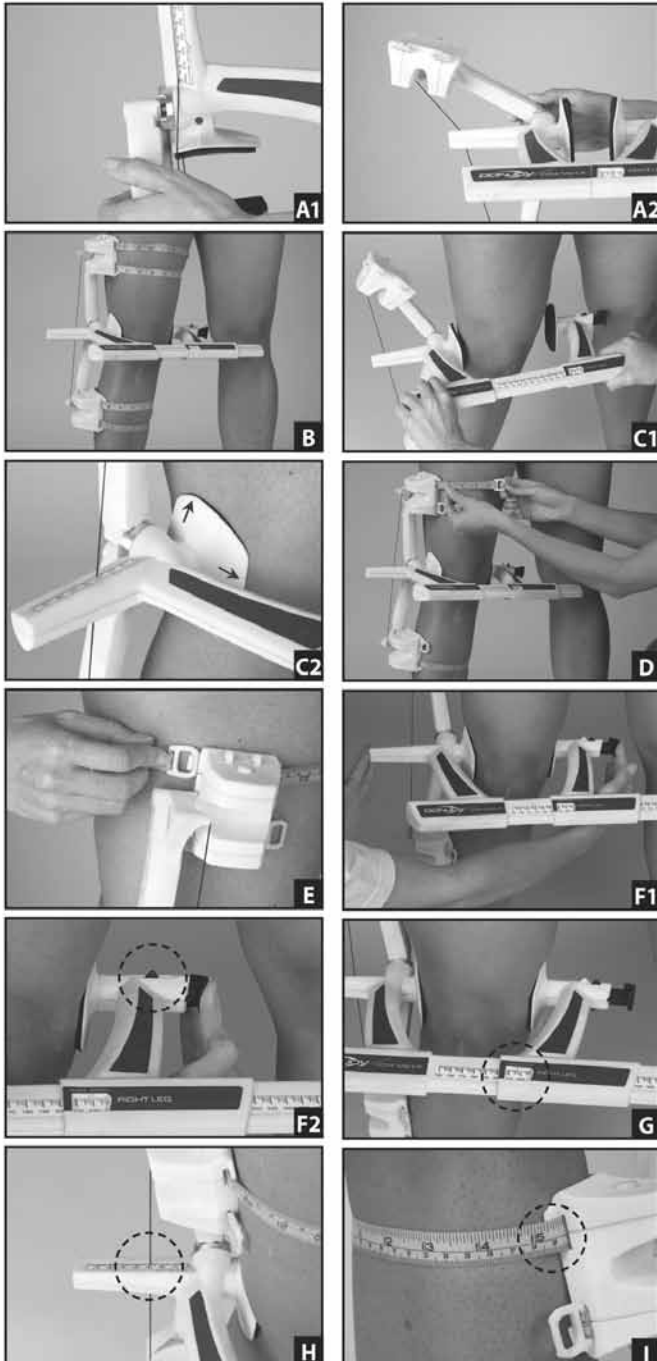

#### APPLICATION INFORMATION:

1. To unstow, distract and rotate swing arms as shown in figures (A1 and A2).
2. Have the patient stand feet shoulder width apart and knees flexed slightly. Do not allow the knees to flex beyond 15 degrees. Apply the instrument directly to the bare leg. Note: Taking measurements from the uninvolved leg is not recommended because of differences in leg dimensions due to dominance of one leg over the other. See figure B.
3. Distract knee width caliber and position on the patient's knee. Arrows on condyle shells should align with the top of the knee cap and slightly posterior to midline. See figures (C1 and C2).
4. For standard thigh and calf, extend tape measure marked in Inches located distal to knee. Wrap around leg and secure to hook on tape module. Press tape release button to pull tape snug to leg; ensure it is parallel to floor. For short thigh or calf, follow same procedure using Metric measurements. See figure (D and E).
5. To establish proper knee compression for knee width measurement, support lateral side of instrument and press load plunger on medial condyle until triangles are aligned, as shown in figures (F1 and F2).
6. Record knee width on order form. See figure (G.)
7. Record lateral offset on order form. See figure (H).
8. Record thigh and calf circumference on order form. See figure (I).